


Use this guide to get to know your meter, and follow steps inside to get started.

IMPORTANT: Please read the Owner's Booklet that came with your system.

Meter icons

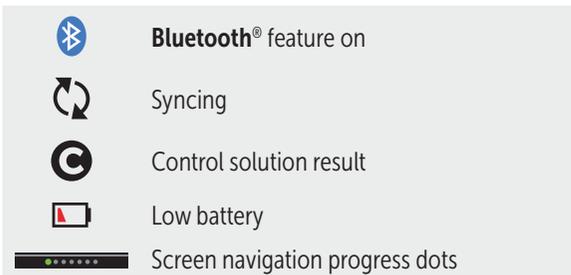

Refer to the Owner's Booklet for meter symbols and icons and their meanings.

Call OneTouch® Customer Care on 0800 121 200 (UK) or 1800 535 676 (Ireland). Lines open 9am-5pm Monday - Friday. www.myOneTouch.co.uk.

LifeScan Europe GmbH
Gubelstrasse 34
6300 Zug
Switzerland

OneTouch®
AW 07202001C
© 2018 - 2021 LifeScan
IP Holdings, LLC
Rev. Date: 10/2021

CE
0344

1 Set up meter

Turn on meter

Press and hold until the Welcome screen appears.

Use or buttons to edit each setting and press to confirm.

Set language


Highlight the language you want and press .



Optional: Complete setup using the OneTouch Reveal® Mobile App*

Select **Yes** to have the App walk you through setup.


Download the OneTouch Reveal® Mobile App before pairing your meter and mobile device.



Set time


Press if the time is correct or edit and confirm.

* Visit www.myOneTouch.co.uk to learn more about the OneTouch Reveal® Mobile App and if available in your country.



Set date

Press if the date is correct or edit and confirm.




Set mealtime range limits

Press if the pre-set Before Meal and After Meal range limits are correct or edit and confirm.



Set Test Tracker


Press if the pre-set goal is correct or edit and confirm.



Set 90 Day Average Target

Press if the 90 Day Average Target is correct or edit and confirm.

NOTE: Talk to your healthcare professional about the right range limits, Daily Test Goal, and 90 Day Average Target for you.



2 Take a test

Wash your hands with soap and warm water, rinse and dry before sampling. Remove the lancing device cap then insert a sterile lancet. Twist the protective cover. Place the cap back onto the device.


Insert a test strip (gold side and 2 silver prongs facing you) to turn the meter on.

Adjust the depth setting on the lancing device. Cock the lancing device and hold firmly against the side of your finger. Press the release button. Gently squeeze finger to get a round drop of blood.

Apply blood sample to the channel on either side of the test strip. Once the channel fills, it will turn red and your result will appear in about 5 seconds.




Silver prongs



Test strip port



Approximate size




Apply Blood

3 View your reading

ColourSure® Dynamic Range Indicator

The ColourSure® Dynamic Range Indicator instantly lets you know if your reading is below (blue), within (green) or above (red) your range limits. It also shows when your reading is near the low or high end of your target range. A text note or emoji points to a segment on the Colour Bar.

Examples of Readings

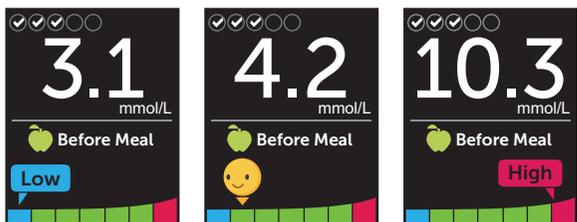

Below Range Low End of Range Above Range

Meal and event tagging


A Before Meal (🍏) tag will automatically be applied to your result. You may change your meal tag to After Meal (🍏) and add an Event tag.



Blood Sugar Mentor™ Messages

The Blood Sugar Mentor™ provides insight on how you're doing and diabetes management guidance, including educational and motivational messages based on your current and previous glucose results and other tracked data.

Examples of Blood Sugar Mentor™ Messages

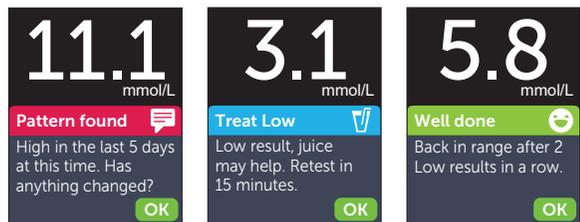


Insight Guidance Encouragement

The **Bluetooth®** word mark and logos are registered trademarks owned by Bluetooth SIG, Inc., and any use of such marks by LifeScan Scotland Ltd. is under licence. Other trademarks and trade names are those of their respective owners.

4 Connect to a mobile device

Bluetooth® technology lets you wirelessly send your readings to a mobile device where you can use the OneTouch Reveal® Mobile App to review and graph your results, set Daily Test Goals, see Blood Sugar Mentor™ Messages and help identify patterns.


On the Settings Menu, highlight **Bluetooth** and press (OK).



A ✓ notes if **Bluetooth®** is currently set to On or Off. Press (↑) or (↓) to change **Bluetooth®** status to On and press (OK).



When prompted by your mobile device, enter the PIN shown.



Example PIN

Register your meter for help and support: myonetouch.co.uk/welcome



ONETOUCH
Verio Reflect®

Blood Glucose Monitoring System

Quick Start Guide



AW 07202001C